

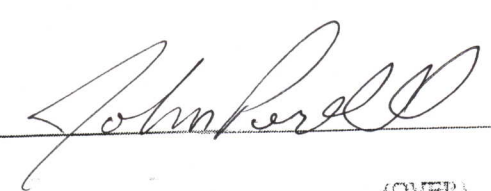
VERIFICATION OF CALIBRATION REPORT

FEB 25 2010

of DataMaster cdm Breath Test Instrument

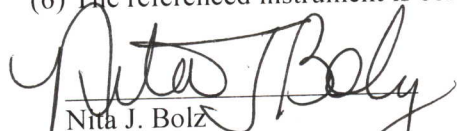
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure		DataMaster cdm S/N	130121 ✓
Name	John Pernell	ID#	6260 Date 2/24/10 ✓
Agency	Fairbanks Airport Police & Fire	Phone #	974-2555
Instrument Location	5195 Brumbaugh Ave. Fairbanks, AK 99709 ✓		
Also S/N		Target Value	High Pressure
X124670 ✓		.082 ✓	1050 psi.
Also Test Values		1 st Also	2 nd Also
.079 ✓		.079 ✓	
Signature			
(OVER)			

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 23rd day of March 2010.


 (Notary Seal Stamp)

Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office

